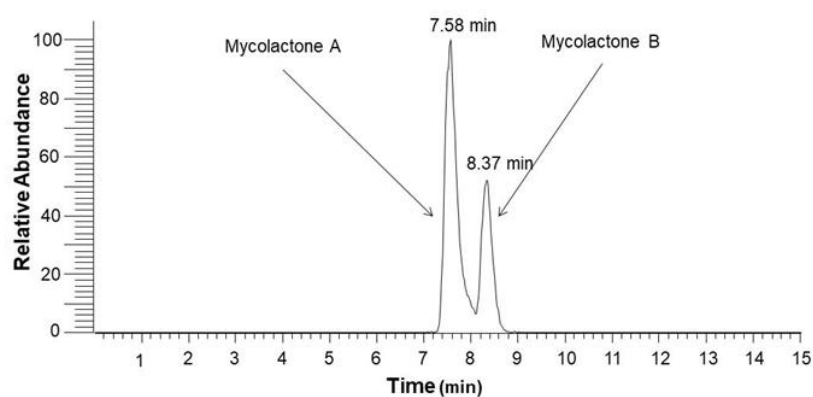
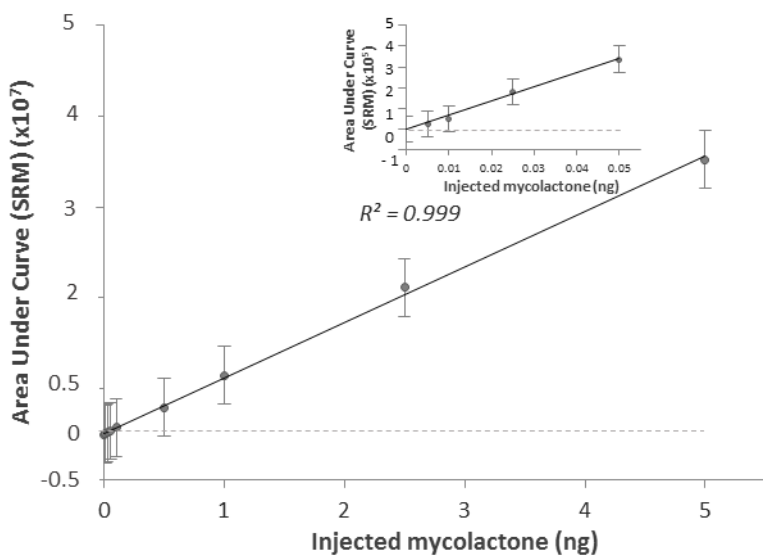


A**B**

Supplementary figure 1: Detection and quantification of mycolactone by liquid chromatography coupled to tandem mass spectrometry

(A) Total ion current (TIC) for mycolactone A/B in selected reaction monitoring (SRM) (MS/MS: 765.5/429.2 UMA) (B) calibration curve.