

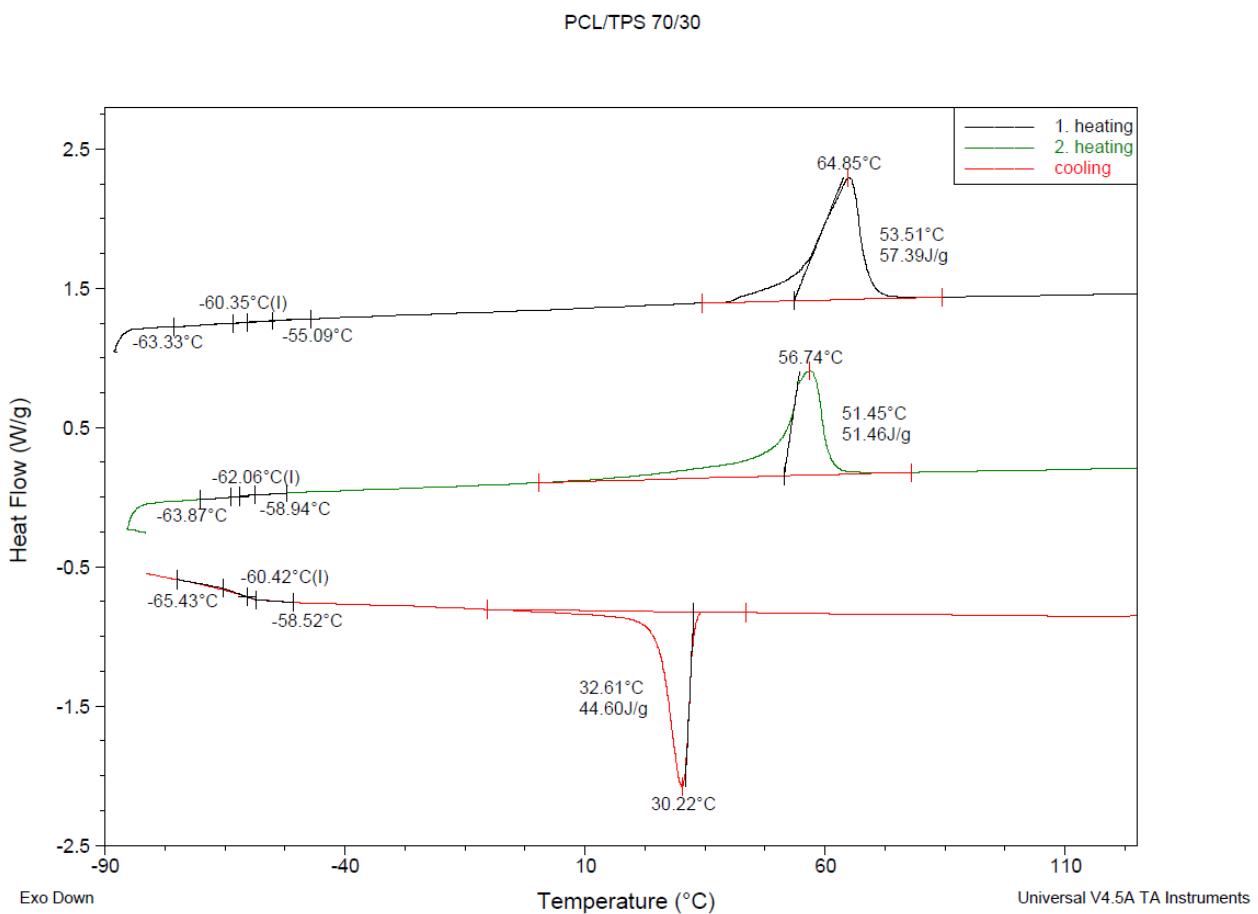


Supplementary: Differential scanning calorimetry results of the PCL/TPS samples.

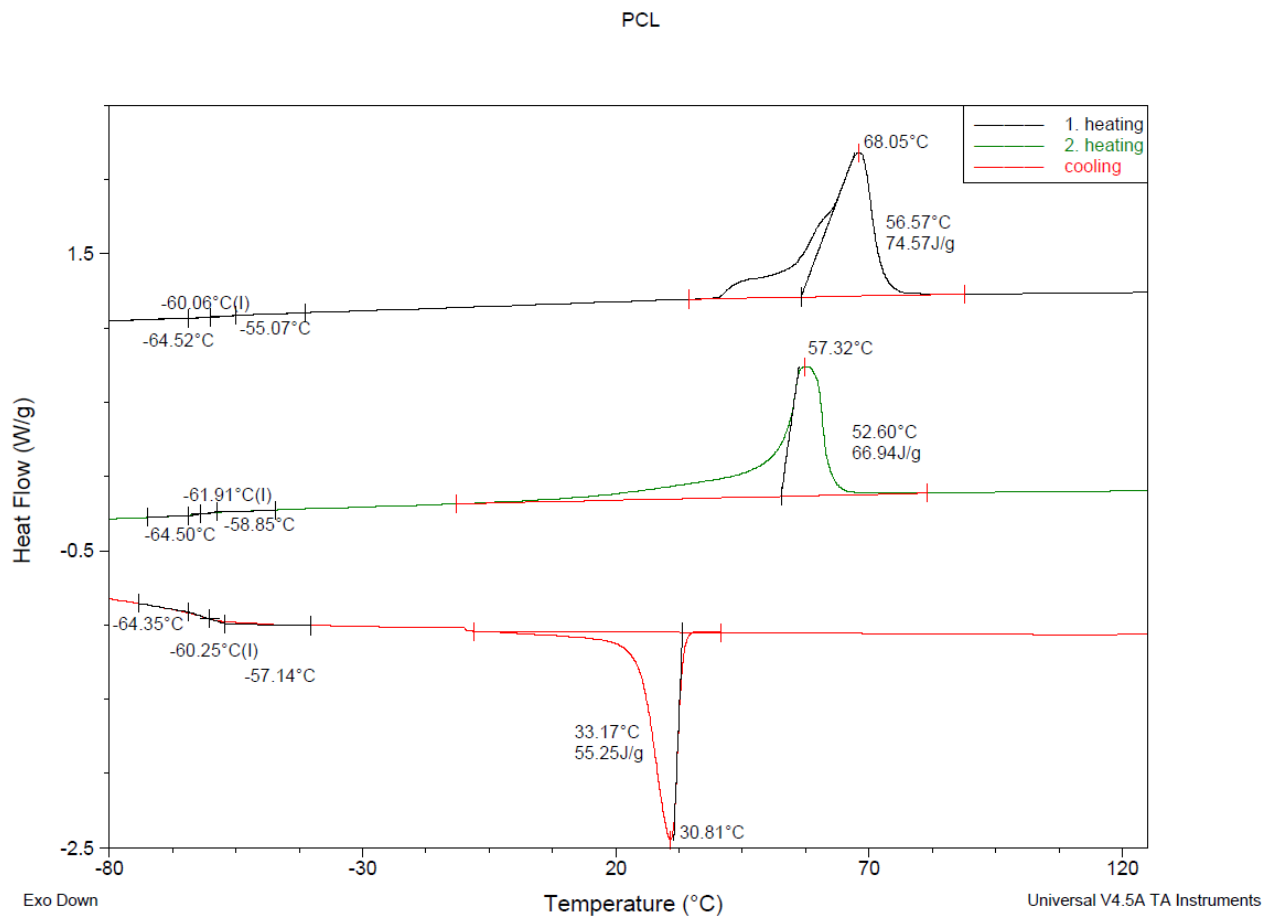

PCL/TPS 50/50

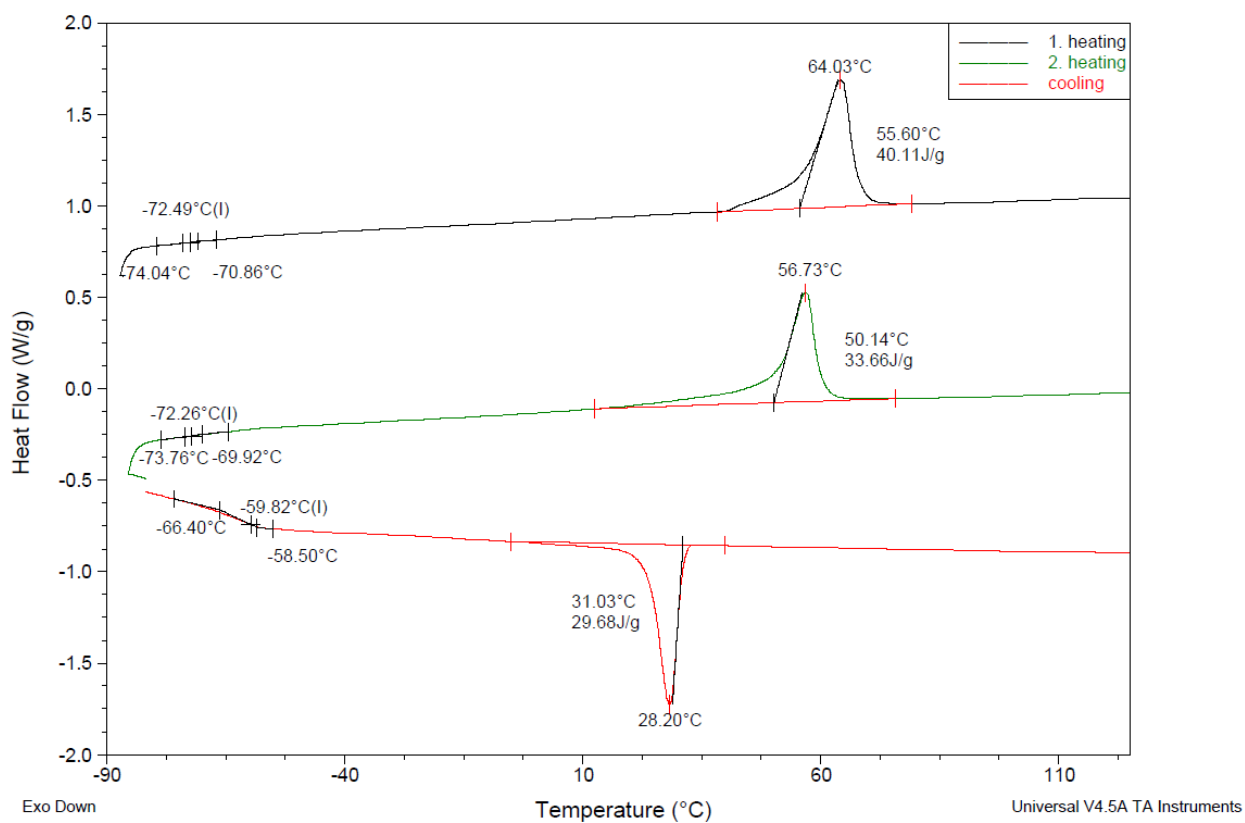

PCL/TPS 30/70

