



A

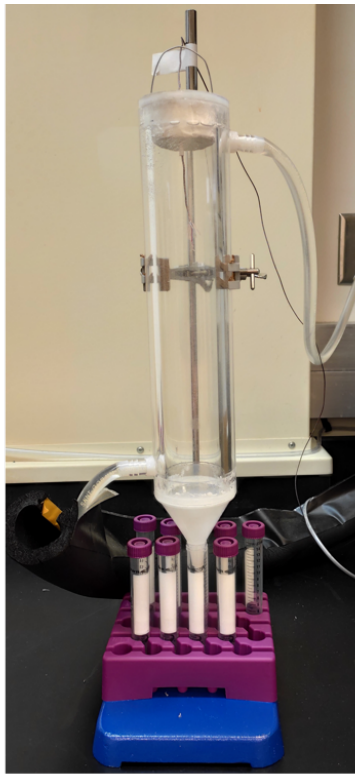

B

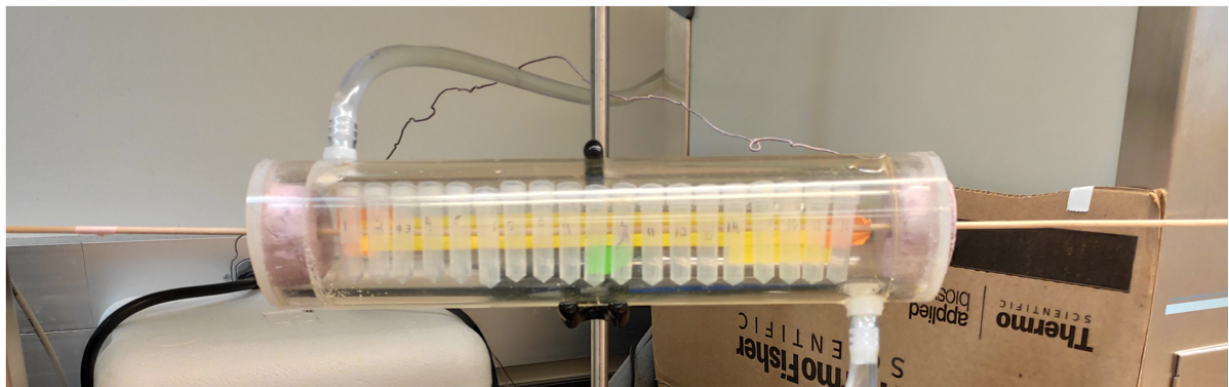

Supplementary Figure 1. Photograph of apparatus for (A) CT_{min} and (B) CT_{max} assays.